

General Specifications

Model FLXA21 2-Wire Analyzer

GS 12A01A02-01E

■ General

The model FLXATM21 2-Wire Analyzer, one model of FLEXATM series, offers single or dual sensor measurement. The modular-designed analyzer offers 4 kinds of measurements – pH/ORP (oxidation-reduction potential), contacting conductivity (SC), inductive conductivity (ISC) or dissolved oxygen (DO) – with the respective sensor module.

For dual sensor measurement, the combination of two same type sensor inputs – pH/ORP and pH/ORP, SC and SC, and DO and DO – are available with two sensor modules. Dual sensor measurement offers additional functionalities; calculated data function and redundant system.

Variety of calculated data from two measuring parameters is selectable for each measurement. On the redundant system built on two measuring parameters of two sensor inputs, main output parameter is automatically switched over to the second sensor output in case of the main sensor's failure condition.



In the FLXA21 Human Machine Interface (HMI), 2-wire type analyzer FLXA21 offers easy touch screen operation and simple menu structure in 12 languages. Menus of display, execution and setting are displayed in a selected language.

The analyzer FLXA21 automatically recognizes the installed sensor module and prepares the necessary menus for right configuration, even for dual sensor measurement.

For immediate measurement, the FLXA21 offers quick setup functionality. The quick setup screen appears when the analyzer is powered. Only a few setups – date/time, language, basic sensor configurations and output – will start the measurement.

The FLXA21 offers the best accuracy in measurement with temperature compensation functionality and calibration functionality. Sensor diagnostics and sensor wellness indication make measurement reliable. Logbook of events and diagnostic data is a useful information source for maintenance.

For hazardous location, the FLXA21 has approvals of ATEX, IECEx, FM, CSA, NEPSI and KCs.

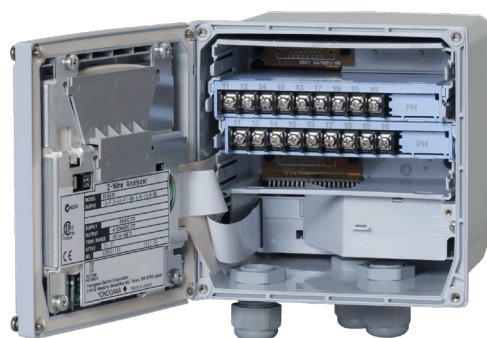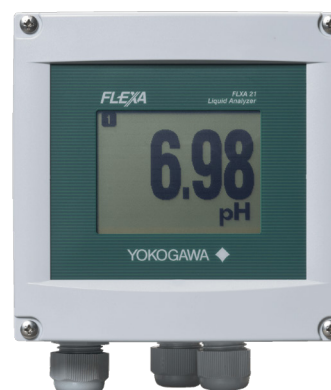

■ Features

- 4 kinds of measurements; pH/ORP, SC, ISC and DO
- Dual sensor measurement on 2-wire type analyzer; pH/ORP and pH/ORP, SC and SC, and DO and DO
- Calculated data from dual sensor measurement
- Redundant system on dual sensor measurement
- Easy touch screen operation on 2-wire type analyzer
- Simple HMI menu structure in 12 languages
- Quick setup menu for immediate measurement
- Indication of sensor wellness
- Hazardous location approvals – ATEX, IECEx, FM, CSA, NEPSI and KCs

FLEXA, FLXA are trademarks or registered trademarks of Yokogawa Electric Corporation.

All other company and product names mentioned in this document are trademarks or registered trademarks of their respective companies.

Please select appropriate equipment in accordance with the laws and regulations of the relevant country/region, when it is used in a location where explosive atmospheres may be present.

■ General Specifications

1. Basic

■ Measurement Object/Sensor Type

- pH/Oxidation-reduction Potential (pH/ORP)
- Conductivity (SC)
- Inductive Conductivity (ISC)
- Dissolved Oxygen (DO)

Note: The available measurement object depends on a sensor module installed on the analyzer.

■ Analyzer Structure

Module structure

● Composition of Analyzer

One (1) Housing assembly
One (1) or two (2) Sensor modules

● Combination of Sensor Module when two modules are installed

Combinations of two same sensor modules are available;

pH/ORP and pH/ORP
SC and SC
DO and DO

2. Measurement

2-1. pH/Oxidation-reduction Potential (pH/ORP)

■ Input Specification

Dual high impedance input ($\geq 10^{12} \Omega$)

■ Input Range

pH: -2 to 16 pH
ORP: -1500 to 1500 mV
rH: 0 to 100 rH

Temperature:

Pt1000: -30 to 140 °C
Pt100: -30 to 140 °C
6.8k: -30 to 140 °C
PTC10k: -30 to 140 °C
NTC 8k55: -10 to 120 °C
3k Balco: -30 to 140 °C
PTC500: -30 to 140 °C

■ Output Range

pH: min. span 1 pH
max. span 20 pH
ORP: min. span 100 mV
max. span 3000 mV
rH: min. span 2 rH
max. span 100 rH
Temperature: min. span 25 °C
max. span 170 °C

■ Performance (Accuracy)

(The specifications are expressed with simulated inputs.)

pH

Linearity: ± 0.01 pH
Repeatability: ± 0.01 pH
Accuracy: ± 0.01 pH

ORP

Linearity: ± 1 mV
Repeatability: ± 1 mV
Accuracy: ± 1 mV

Temperature

with Pt1000, 6.8k, PTC10k, NTC 8k55, 3k Balco, PTC500

Linearity: ± 0.3 °C
Repeatability: ± 0.1 °C
Accuracy: ± 0.3 °C

with Pt100

Linearity: ± 0.4 °C
Repeatability: ± 0.1 °C
Accuracy: ± 0.4 °C

2-2. Conductivity (SC)

■ Input Specification

Two or four electrodes measurement with square wave excitation, using max 60m (200ft) cable (WU40/ WF10) and cell constants from 0.005 to 50.0 cm^{-1}

■ Input Range

Conductivity:

min.: 0 $\mu\text{S}/\text{cm}$
max.: 200 mS x (Cell constant)
(over range 2000 mS/cm)

Resistivity:

min.: 0.005 k Ω / (Cell constant)
max.: 1000 M Ω x cm

Temperature:

Pt1000: -20 to 250 °C
Pt100: -20 to 200 °C
Ni100: -20 to 200 °C
NTC 8k55: -10 to 120 °C
Pb36(JIS NTC 6k): -20 to 120 °C

■ Output Range

Conductivity:

min. 0.01 $\mu\text{S}/\text{cm}$
max. 2000 mS/cm (max 90% zero suppression)

Resistivity:

min. 0.001 k Ω x cm
max. 1000 M Ω x cm (max 90% zero suppression)

Temperature:

min. span 25 °C
max. span 270 °C

■ Performance (Accuracy)

(The specifications are expressed with simulated inputs.)

Conductivity

2 $\mu\text{S} \times \text{K cm}^{-1}$ to 200 mS x K cm^{-1}
Accuracy: $\pm 0.5\%$ F.S.
1 $\mu\text{S} \times \text{K cm}^{-1}$ to 2 $\mu\text{S} \times \text{K cm}^{-1}$
Accuracy: $\pm 1\%$ F.S.

Resistivity

0.005k Ω / K cm^{-1} to 0.5M Ω / K cm^{-1}
Accuracy: $\pm 0.5\%$ F.S.
0.5M Ω / K cm^{-1} to 1M Ω / K cm^{-1}
Accuracy: $\pm 1\%$ F.S.

Temperature

with Pt1000, Pb36, Ni100
Accuracy: ± 0.3 °C
with Pt100, NTC 8k55
Accuracy: ± 0.4 °C

Temperature compensation

NaCl table: ± 1 %
Matrix: ± 3 %

Step response: 90 % (< 2 decades) in 7 seconds

Note: "F.S." means maximum setting value of analyzer output.

"K" means cell constant.

YOKOGAWA provides conductivity sensors of which cell constants are 0.1 to 10 cm^{-1} .

2-3. Inductive Conductivity (ISC)

■ Input Specification

Compatible with the Yokogawa inductive conductivity ISC40 series with integrated temperature sensor: NTC30k or Pt1000.

■ Input Range

Conductivity: 0 to 2000 mS/cm at 25 °C reference temperature.
 Temperature: -20 to 140 °C
 Cable length:
 max. 60 meters total length of fixed sensor cable + WF10(J) extension cable.
 Influence of cable can be adjusted by doing an AIR CAL with the cable connected to a dry cell.

■ Output Range

Conductivity:
 min. span: 100 μ S/cm
 max. span: 2000 mS/cm (max 90% zero suppression)
 Temperature:
 min. span 25 °C
 max. span 160 °C

■ Performance (Accuracy)

(The specifications are expressed with simulated inputs.)

(Output span is 0-100 μ S/cm or more)

Conductivity:
 Linearity: $\pm(0.4 \% \text{F.S.} + 0.3 \mu\text{S/cm})$
 Repeatability: $\pm(0.4 \% \text{F.S.} + 0.3 \mu\text{S/cm})$
 Temperature: $\pm 0.3 ^\circ\text{C}$
 Step response: 90 % (< 2 decades) in 8 seconds
 Note: "F.S." means maximum setting value of analyzer output.

2-4. Dissolved Oxygen (DO)

■ Input Specification

The FLXA21 accepts output from membrane covered Dissolved Oxygen sensors. These sensors can be Galvanic type, where the sensor generates its own driving voltage or Polarographic type, where the sensor uses external driving voltage from the converter.

The input range is 0 to 50 μ A for Galvanic sensors and 0 to 1 μ A for Polarographic sensors.
 For temperature compensation, the FLXA21 accepts Pt1000 (DO30 sensor) and NTC22k elements (OXYFERM and OXYGOLD sensors).

■ Input Range

Dissolved Oxygen: 0 to 50 mg/l (ppm)
 Temperature: -20 to 150 °C
 DO30G sensor:
 Measurement range: 0 to 20 mg/l (ppm)
 Temperature: 0 to 40 °C
 Hamilton sensors:
 Oxyferm:
 Measurement range: 10 ppb to 40 ppm
 Temperature range: 0 to 130 °C
 Oxygold G:
 Measurement range: 2 ppb to 40 ppm
 Temperature range: 0 to 130 °C
 Oxygold B:
 Measurement range: 8 ppb to 40 ppm
 Temperature range: 0 to 100 °C

■ Output Range

DO concentration:
 mg/l (ppm):
 min.: 1 mg/l (ppm)
 max.: 50 mg/l (ppm)
 ppb:
 min.: 1 ppb
 max.: 9999 ppb
 % saturation:
 min.: 10 %
 max.: 600 %
 Temperature:
 min. span 25 °C
 max. span 170 °C

■ Performance (Accuracy)

(The specifications are expressed with simulated inputs.)

Performance in ppm mode:

Linearity: $\pm 0.05 \text{ ppm}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Repeatability: $\pm 0.05 \text{ ppm}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Accuracy: $\pm 0.05 \text{ ppm}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Performance in ppb mode:

Linearity: $\pm 1 \text{ ppb}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Repeatability: $\pm 1 \text{ ppb}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Accuracy: $\pm 1 \text{ ppb}$ or $\pm 0.8 \% \text{ F.S.}$, whichever is greater

Temperature

Linearity: $\pm 0.3 ^\circ\text{C}$

Repeatability: $\pm 0.1 ^\circ\text{C}$

Accuracy: $\pm 0.3 ^\circ\text{C}$

Note: "F.S." means maximum setting value of analyzer output.

3. Electrical

■ Output Signal

General: One output of 4-20 mA DC
 Note: Tolerance: $\pm 0.02 \text{ mA}$
 Bi-directional HART digital communication, superimposed on mA (4-20mA) signal

Output function:

Linear or Non-linear (21-step table)

Burn out function: (NAMUR 43 except ISC)

Without HART/PH201G:

Down: 3.6 mA

(signal: 3.8 to 20.5 mA for pH/ORP, SC and DO)

(signal: 3.9 to 20.5 mA for ISC)

Up: 22mA

With HART/PH201G:

Down: 3.6 mA for pH/ORP, SC and DO

Down: 3.9 mA for ISC

(signal: 3.8 to 20.5 mA for pH/ORP, SC and DO)

(signal: 3.9 to 20.5 mA for ISC)

Up: 22mA

■ Power Supply

Nominal 24 V DC loop powered system

One (1) Sensor module (1 input):

16 to 40V DC (for pH/ORP, SC and DO)

17 to 40V DC (for ISC)

Two (2) Sensor modules (2 inputs):

22.8 to 40V DC (for pH/ORP, SC and DO)

Note: When the FLXA21 is used in the multi-drop mode of HART communication, the output signal is changed from 12.5 mA DC to 4 mA DC just after the power is turned on. Enough power supply for the instruments is to be provided.

● Maximum Load Resistance

Refer to the Figure 1.

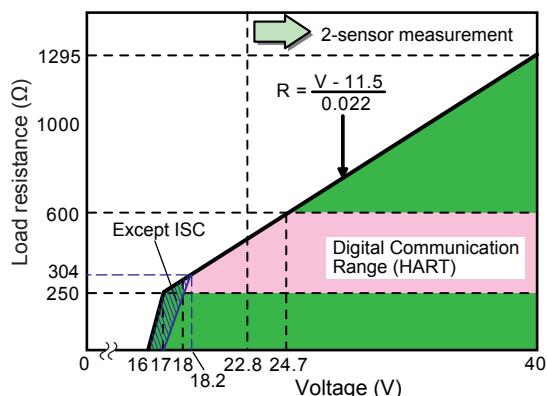


Figure 1 Supply Voltage and Load Resistance

■ Display

LCD with a touch screen:

Black/White: 213 x 160 pixels

Contrast adjustment available on the touch screen

Message language:

12 (English, Chinese, Czech, French, German, Italian, Japanese, Korean, Polish, Portuguese, Russian and Spanish)
One analyzer has all 12 languages.

Note: Description for a selection of language and language names are written in English.

Note: Only English alphabet and numeric are available for a tag number, an additional description for each value on the display screen and passwords.

Note: Only for message language on the screen, 12 languages are provided.

4. Mechanical and others

■ Housing

Case: Plastic (Polycarbonate)

Case color and finish:

Color: Silver gray (equivalent to Munsell 3.2PB7.4/1.2)

Window: Polycarbonate (flexible)

Protection: IP66 (except Canada), NEMA Type 4X (USA), CSA Type 3S/4X (Canada)

■ Plate

Main name plate: inside case cover

Regulation plate:

on the case outside

■ Cable and Terminal

Cable size:

Outer diameter:

6 to 12 mm (suitable for M20 cable gland)

3.4 to 7 mm (grounding cable for plastic case)

Terminal screw size: M4

torque of screw up: 1.2 N•m

Wire terminal:

Pin terminal, ring terminal and spade terminal can be used for analyzer's power supply terminals and sensor terminals.

Pin terminal: pin diameter: max. 1.9 mm

Ring and spade terminal: width: max. 7.8 mm

■ Cable Entry

1-Sensor measurement:

3 holes,

M20 cable gland x 3 pcs,

Sleeve x 1 pc (for grounding cable line)

2-Sensor measurement:

4 holes,

M20 cable gland x 4 pcs,

Sleeve x 1 pc (for grounding cable line)

Note: Cable glands are delivered with an analyzer, but not assembled into the analyzer.

■ Mounting

Mounting hardware (option):

- Universal mounting kit (Note)
- Pipe and wall mounting hardware
- Panel mounting hardware

Note: This kit contains the pipe and wall mounting hardware and the panel mounting hardware.

Hood (option):

- Stainless steel
- Stainless steel with urethane coating
- Stainless steel with epoxy coating

■ Stainless Steel Tag Plate

When the additional code "/SCT" with a tag number is specified, the tag plate on which the tag number is inscribed is delivered with the analyzer.

Tag plate is hanging type.

■ Conduit Adapter

Using optional adapter

- G1/2 (quantity: 4)
- 1/2NPT (quantity: 4)
- M20 x 1.5 (quantity: 4)

These conduit adapters are delivered with an analyzer, but not assembled into the analyzer.

■ Size of Housing Case

144 (W) x 144 (H) x 151 (D) mm (without cable gland)

■ Weight

Approx. 1 kg

■ Ambient Operating Temperature

-20 to +55 °C

■ Storage Temperature

-30 to +70 °C

■ Humidity

10 to 90% RH at 40°C (Non-condensing)

5. Digital Communication

■ Kind of Digital Communication

- HART (HART 5) or PH201G dedicated distributor

Note: Only one kind of digital communication is available for one analyzer.

■ Output Value Parameter (HART)

Four value parameters (measured values) are available for one digital communication.

- For 1-sensor measurement, these parameters are measured values.
- For 2-sensor measurement, refer to the next item.

■ Digital Communication of 2-Sensor Measurement (HART)

Even when two sensor modules are installed, only one digital communication is available for 2-sensor measurement.

Four value parameters can be selected from the followings;

- Measured values of two sensors
- Calculated data of 2-sensor measurement
- Redundant system output

■ Specific Contact Output with dedicated distributor, model PH201G

The distributor, model PH201G, is designed to connect with the 2-Wire Analyzer.

This distributor supplies drive power to the analyzer and receives simultaneously 4-20 mA DC signal from the analyzer.

This signal is converted to 1-5 V DC signal in the distributor.

This distributor also receives digital signals superimposed on the 4-20 mA DC signal, and provides contact outputs

Input/Output signal:

- Number of available drive/signal point: 1
- Output signal: 1-5 V DC (2 points) (Note)
- Load resistance: 2 k Ω or less (1-5 V DC output)
- Isolation system: Loop isolation type
- Note: Two output signals for one analyzer's analog output are provided. Two 1-5 V DC output signals are same.

Contact output:

Contact rating:

- 250 V AC, maximum 100 VA
- 220 V DC, maximum 50 VA

Hold contact output:

- NC contact, normally energized
- Contact closes when power is off or during Hold situation.

Fail contact output:

- NC contact, normally energized
- Contact closes when power is off or during Fail/Warning conditions.

Wash contact output:

- NO contact
- Contact closes during wash cycles.

■ Regulatory Compliance (FLXA21)

■ Safety, EMC and RoHS Compliance

- Safety: UL 61010-1
UL 61010-2-030
NM EN 61010 1, NM EN 61010 2 030
GB30439 Part 1
CAN/CSA C22.2 No.61010-1
CAN/CSA-C22.2 No.61010-2-030
EN 61010-1
EN IEC 61010-2-030
- EMC: EN 61326-1 Class A, Table 2 (For use in industrial locations)
EN 61326-2-3
NM EN 61326 1, NM EN 61326 2 3
RCM: EN 61326-1 Class A, Table 2
Korea Electromagnetic Conformity Standard Class A 한국 전자파적합성 기준
Russian: TR CU 020/2011

RoHS: EN IEC 63000 (Style 3.06 and later)

Installation altitude: 2000 m or less

Category based on IEC 61010: I (Note 1)

Pollution degree based on IEC 61010: 2 (Note 2)

Note 1: Installation category, called over-voltage category, specifies impulse withstand voltage. Equipment with "Category I" (ex. two wire transmitter) is used for connection to circuits in which measures are taken to limit transient over-voltages to an appropriately low level.

Note 2: Pollution degree indicates the degree of existence of solid, liquid, gas or other inclusions which may reduce dielectric strength. Degree 2 is the normal indoor environment.

Information of the WEEE Directive

This product is purposely designed to be used in a large scale fixed installations only and, therefore, is out of scope of the WEEE Directive. The WEEE Directive does not apply. The WEEE Directive is only valid in the EU.

REACH: Regulation EC 1907/2006

■ Explosion Protected Type Compliance

Item	Description	'Type' in MS code
Europe (ATEX)	[Intrinsic safety "ia"] Applicable Standard: EN IEC 60079-0, EN 60079-11 Certificate No: DEKRA 11ATEX0109X Marking/Rating:  II 1 G Ex ia IIC T4 Ga Ambient Temperature: -20 to 55°C Power Supply / Signals: See the control drawing. Electrical parameters: See the control drawing. Dielectric strength: 500 V a.c. r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V d.c. between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: Electrostatic charges on the non-metallic or coated parts of the two wire analyzer shall be avoided. Since the enclosure of the Model FLXA202 is made of aluminium, if it is mounted in an area where the use of EPL Ga (category 1 G) equipment is required, it shall be installed such that, even in the event of rare incidents, ignition sources due to impact and friction sparks are excluded. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (1)	-CB
International (IECEx)	[Intrinsic safety "ia"] Applicable Standard: IEC 60079-0, IEC 60079-11 Certificate No: IECEx DEK 11.0044X Marking/Rating: Ex ia IIC T4 Ga Ambient Temperature: -20 to 55°C Power Supply / Signals: See the control drawing. Electrical parameters: See the control drawing. Dielectric strength: 500 V a.c. r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V d.c. between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: Electrostatic charges on the non-metallic or coated parts of the two wire analyzer shall be avoided. Since the enclosure of the Model FLXA202 is made of aluminium, if it is mounted in an area where the use of EPL Ga (category 1 G) equipment is required, it shall be installed such that, even in the event of rare incidents, ignition sources due to impact and friction sparks are excluded. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (1)	


Item	Description	'Type' in MS code
United States (FM)	[Intrinsically safe / Nonincendive] Applicable Standard: FM 3600, FM3610, FM3611, FM3810, NEMA 250, ANSI/UL 60079-0, ANSI/UL 60079-11, ANSI/UL 121201, ANSI/UL 61010-1, ANSI/UL 61010-2-030 Certificate No: FM20US0046X Marking/Rating: IS CL I DIV 1 GP ABCD T4, CL I ZN 0 AEx ia IIC T4 NI CL I DIV 2 GP ABCD T4, CL I ZN 2 IIC T4 T4: for ambient temperature: -20 to 55°C Enclosure: Type 4X Power Supply / Signals: See the control drawing. Battery: No replaceable batter Electrical parameters: See the control drawing. Dielectric strength: 500 V AC, r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V DC between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: See the control drawings. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (3)	-CD
Canada (FM)	[Intrinsically safe / Nonincendive] Applicable Standard: CAN/CSA-C22.2 No.94.2, CAN/CSA-C22.2 No.213, CSA-C22.2 No.60079-0, CAN/CSA-C22.2 No.60079-11, CAN/CSA-C22.2 No.61010-1, CAN/CSA-C22.2 No.61010-2-030 Certificate No: FM23CA0014X Marking/Rating: Ex ia IIC T4 Ga Intrinsically safe for Class I, Division 1, Groups A, B, C, D, T4 Nonincendive for Class I, Division 2, Groups A, B, C, D, T4 Ambient Temperature: -20 to 55°C Ambient Humidity: 0 – 100% (No Condensation) Enclosure: Type 4X Power Supply / Signals: See the control drawing. Electrical parameters: See the control drawing. Dielectric strength: 500 V AC, r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V DC between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: See the control drawings. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (2)	

Item	Description	'Type' in MS code
United States (FM)	[Nonincendive] Applicable Standard: FM 3600, FM3611, FM3810, NEMA 250, ANSI/UL 121201, ANSI/UL 61010-1, ANSI/UL 61010-2-030 Certificate No: FM20US0046X Marking/Rating: NI CL I DIV 2 GP ABCD T4, CL I ZN 2 IIC T4 T4: for ambient temperature: -20 to 55°C Enclosure: Type 4X Power Supply / Signals: See the control drawing. Battery: No replaceable batter Electrical parameters: See the control drawing. Dielectric strength: 500 V AC, r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V DC between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: See the control drawings. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (3)	-DD
Canada (FM)	[Nonincendive] Applicable Standard: CAN/CSA-C22.2 No.94.2, CAN/CSA-C22.2 No.213, CAN/CSA-C22.2 No.61010-1, CAN/CSA-C22.2 No.61010-2-030 Certificate No: FM23CA0014X Marking/Rating: Nonincendive for Class I, Division 2, Groups A, B, C, D, T4 Ambient Temperature: -20 to 55°C Ambient Humidity: 0 – 100% (No Condensation) Enclosure: Type 4X Power Supply / Signals: See the control drawing. Electrical parameters: See the control drawing. Dielectric strength: 500 V AC, r.m.s. between - Supply terminals and the earth terminal - the terminals of Measuring Modules excluding PH, SC and ISC and the earth terminal - Supply terminals and the terminals of Measuring Modules - the terminals of Measuring Module 1 and the terminals of Measuring Module 2 700 V DC between - the terminals of PH, SC and ISC Measuring Modules and the earth terminal Specific conditions of use: See the control drawings. On-site assembling: See Use's Manual IM 12A01A03-01EN. Installation and erection: See the control drawing. Maintenance and Repair: Warning: A modification of the equipment would no longer comply with the construction described in the certificate documentation. Only personnel authorized by Yokogawa Electric Corporation can repair the equipment. Control Drawing: Refer to (2)	
China (NEPSI)	[Intrinsic safety "ia"] Applicable Standard: GB/T 3836.1-2021, GB/T 3836.4-2021 Certificate No: GYJ22.3555X Marking/Rating: Ex ia IIC T4 Ga Ambient Temperature: -20 to 55°C Control Drawing: Refer to (4)	-CH
Korea (KCs)	[Intrinsic safety "ia"] Applicable Standard: Notice of Ministry of Labor No. 2021-22 Certificate No: 21-KA4BO-0915X Marking/Rating: Ex ia IIC T4 Ga Ambient Temperature: -20 to 55°C Control Drawing: Refer to (4)	-EG

■ Control Drawings

(1) ATEX and IECEx Intrinsic safety “ia”

Yokogawa Electric Corporation		FLXA21 / FLXA202			
Title	Control drawing (for 4-20mA type)				
No.	IKF039-A31	Page	1	Revision	0
		Date	2019-10-18		

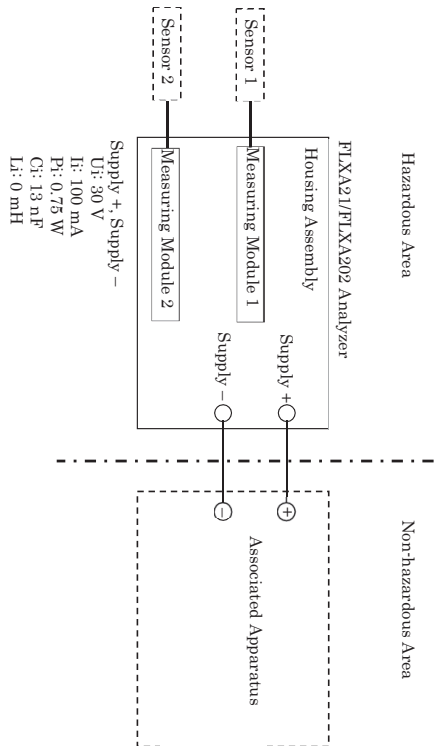

Measuring Module 1, 2

	Type of Measuring Module	
	pH, SC, DO	ISC
Uo	11.76 V	11.76 V
Io	116.5 mA	60.6 mA
Po	0.3424 W	0.178 W
Co	100 nF	100 nF
Lo	1.7 mH	8 mH

Notes:

1. The associated apparatus must be a linear source.
2. "Measuring Module 2" is not always installed.
3. ISC module, SENCOM module and SSA module are not installed as "Measuring Module 2".
4. Sensor 1 and Sensor 2 may be simple apparatus or intrinsically safe apparatus.
5. In case of SSA module, Sensor 1 is SENCOM SA (SENCOM Smart Adaptor).
6. When accessing the display window or other non-metallic parts of the enclosure of FLXA202/FLXA21, take the following measures to minimize the risk of explosion from electrostatic discharges, in addition to avoiding any actions that cause the generation of electrostatic charges, such as rubbing with a dry cloth.

To avoid electrostatic charge on the operator,

- Earth the operator through a wrist-strap, or
- Operate FLXA202/FLXA21 on the conductive floors, wearing anti-static work clothes and electrostatic safety shoes, or
- Neutralize the operator and FLXA202/FLXA21 by a static elimination bar which has a metal part earthed through resistor from 100kΩ to 100MΩ.


In case that those measures cannot be taken or static electricity cannot be suppressed, bring a gas detector and make sure there is no ignition capable atmosphere around FLXA202/FLXA21 before the operation.

(2) US and Canada Intrinsic safety, Nonincendive

Yokogawa Electric Corporation		FLXA21 / FLXA202			
Title	Control drawing (4-20 mA type)				
No.	IFM039-A/71	Page	1	Revision	10
		Date	2022-08-08		

Installation for Division 1 / Zone 0, 1

Applicable models: FLXA21-D-x-x-CD-xx-xx-A-..., FLXA202-D-x-x-CD-xx-xx-A-...

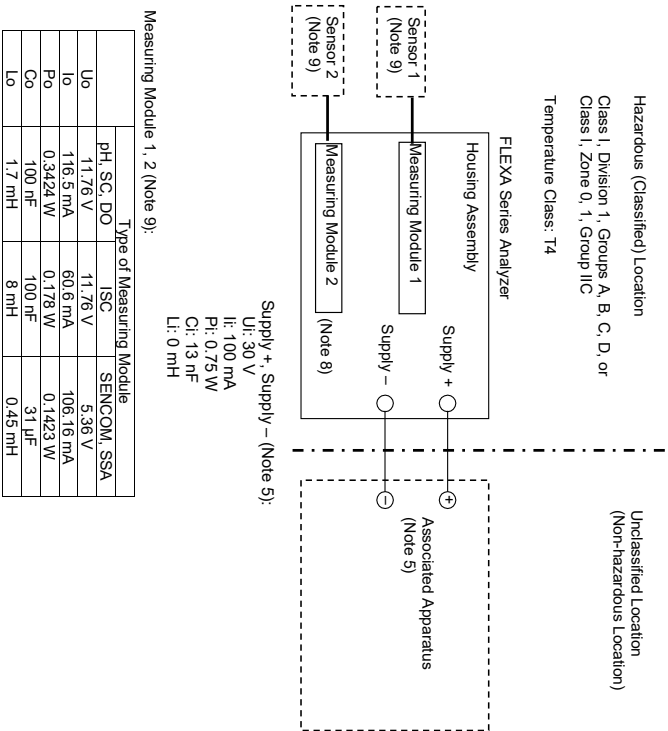


Specific conditions of use:

- Precautions shall be taken to minimize the risk of non-metallic parts and painted parts of the enclosure. When the equipment is used in hazardous locations, avoid any action which generates electrostatic discharge such as rubbing with a dry cloth.
- In the case where the enclosure of the analyzer is made of Aluminum, if it is mounted in ZONE 0, it must be installed such that, even in the event of rare incidents, ignition sources due to impact and friction sparks are excluded.

Yokogawa Electric Corporation		Model			FLXA21 / FLXA202		
Title		Control drawing (4-20 mA type)					
No.	IFM039-A71	Page	2	Revision	10		

Installation for Division 2 / Zone 2

Applicable models: FLXA21-D-x-x-CD-xx-xx-A-..., FLXA21-D-x-x-DD-xx-xx-A-..., FLXA202-D-x-x-CD-xx-xx-A-..., FLXA202-D-x-x-DD-xx-xx-A-...

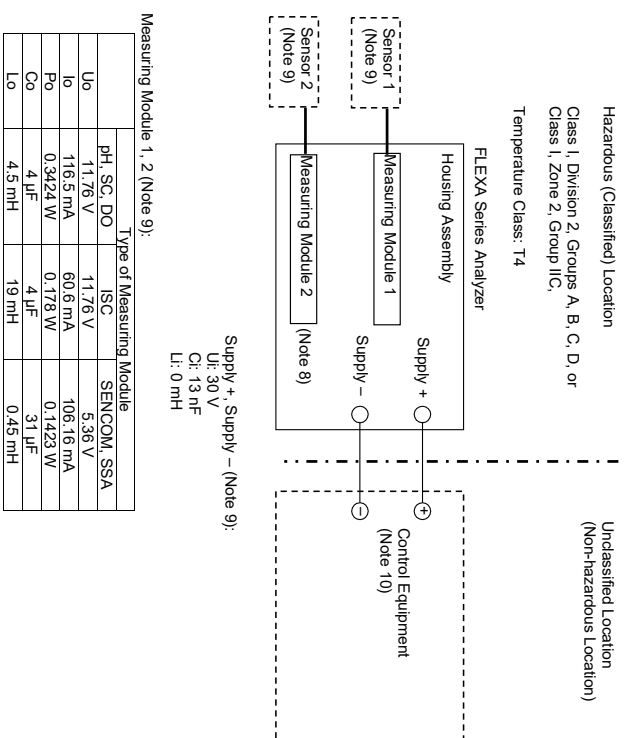

Specific condition of use:

- Precautions shall be taken to minimize the risk of non-metallic parts and painted parts of the enclosure. When the equipment is used in hazardous locations, avoid any action which generates electrostatic discharge such as rubbing with a dry cloth.

Yokogawa Electric Corporation		Model			FLXA21 / FLXA202	
Title		Control drawing (4-20 mA type)				
No.	IFM039-A71	Page	3	Revision	10	

Notes:

- This drawing replaces the former control drawing IKE039-A12.
- No revision to this drawing without prior approval of FM.
- In US, the associated apparatus and the associated nonincendive field wiring apparatus must be FM-approved.
- In US, installation must be in accordance with the National Electric Code (NFPA 70), ANSI/ISA-RP12.06.01 and relevant local codes.
In Canada, installation must be in accordance with the Canadian Electric Code Part I (C22.1), ANSI/ISA-RP12.06.01 and relevant local codes.
- The associated apparatus must be a linear source meeting the following conditions.

$$U_0 \text{ (or } V_{oc}) \leq U_i$$

$$I_0 \text{ (or } I_{sc}) \leq I_i$$

$$P_0 \leq P_i$$

$$C_0 \text{ (or } C_a) \geq C_i + C_{cable}$$

$$L_0 \text{ (or } L_a) \geq L_i + L_{cable}$$
- Control equipment connected to the associated apparatus must not use or generate a voltage which exceeds U_m of the associated apparatus.
- The control drawing of the associated apparatus must be followed when installing the equipment.
- Measuring Module 2 is not always installed.
- ISC module, SENCOM module and SSA module are not installed as "Measuring Module 2".
- When installed in Division 1, Zone 0 or Zone 1, Sensor 1 and Sensor 2 may be simple apparatus or intrinsically safe apparatus meeting the conditions below.
When installed in Division 2 or Zone 2, Sensor 1 and Sensor 2 may be simple apparatus or nonincendive field wiring apparatus meeting the conditions below, or alternatively, they may be equipment suitable for Division 2 or Zone 2 respectively, if a suitable wiring method other than nonincendive field wiring is employed.

$$U_i \text{ (or } V_{max}) \geq U_0$$

$$I_i \text{ (or } I_{max}) \geq I_0$$

$$P_i \geq P_0$$

$$C_i \leq C_0 - C_{cable}$$

$$L_i \leq L_0 - L_{cable}$$
- The control equipment must be the associated nonincendive field wiring apparatus meeting the conditions below. Alternatively, it may be general-purpose equipment, if a suitable wiring method other than nonincendive field wiring is employed.

$$U_0 \text{ (or } V_{oc}) \leq U_i$$

$$C_0 \text{ (or } C_a) \geq C_i + C_{cable}$$

$$L_0 \text{ (or } L_a) \geq L_i + L_{cable}$$

Yokogawa Electric Corporation		Model		FLXA21 / FLXA202	
Title	Control drawing (4-20 mA type)				
No.	IFM039-A71	Page	4	Revision	10

- WARNING – POTENTIAL ELECTROSTATIC CHARGING HAZARD – WHEN THE EQUIPMENT IS USED IN HAZARDOUS LOCATIONS, AVOID ANY ACTION WHICH GENERATE ELECTROSTATIC DISCHARGE SUCH AS RUBBING WITH A DRY CLOTH.
AVERTISSEMENT – DANGER POTENTIEL DE CHARGES ELECTROSTATIQUES.
- WARNING – IN THE CASE WHERE THE ENCLOSURE OF THE ANALYZER IS MADE OF ALUMINUM, IF IT IS MOUNTED IN ZONE 0, IT MUST BE INSTALLED SUCH THAT, EVEN IN THE EVENT OF RARE INCIDENTS, IGNITION SOURCES DUE TO IMPACT AND FRICTION SPARKS ARE EXCLUDED
AVERTISSEMENT - DANS LE CAS OÙ LE BOÎTIER DE L'ANALYSEUR EST EN ALUMINIUM, S'IL EST MONTÉ EN ZONE 0, IL DOIT ÊTRE INSTALLÉ DE MANIÈRE À CE QUE, MÊME EN CAS D'INCIDENTS RARES, LES SOURCES D'INFLAMMATION DUES AUX CHOC ET AUX ÉTINCELLES DE FRICTION SOIENT EXCLUES.
- WARNING – SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY
AVERTISSEMENT – LA SUBSTITUTION DE COMPOSANTS PEUT COMPROMETTRE LA SÉCURITÉ INTRINSÈQUE.
- WARNING – SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY AND SUITABILITY FOR DIVISION 2 / ZONE 2.
AVERTISSEMENT – LA SUBSTITUTION DE COMPOSANTS PEUT COMPROMETTRE LA SÉCURITÉ INTRINSÈQUE.

(3) NEPSI and KCs Intrinsic safety “ia”

(Refer to (1) ATEX and IECEx Control Drawing)

■ Model & Suffix Codes


Model	Suffix code	Option code	Description
FLXA21			2-Wire Analyzer
Power supply	-D		Always -D
Housing	-P		Plastic
Display	-D		Anti-glare LCD
Type	-AB -AD -AG -AQ -AR -CB -CD -CH -EG -EQ -ER -DD		General purpose for CE, RCM General purpose for CSA General purpose for KC General purpose for EAC with PA for Russia. (Note 1) General purpose for EAC (Note 2) IS for ATEX, IEC Ex (Note 3) IS for US, Canada (Note 4) IS for NEPSI (Note 5) IS for KCs (Note 6) IS for EACEx with PA for Russia (Note 7) IS for EACEx (Note 8) NI for US, Canada (Note 9)
1st input	-P1 -C1 -C5 -D1		pH/ORP Conductivity (SC) Inductive conductivity (ISC) Dissolved oxygen (DO)
2nd input (Note 10)	-NN -P1 -C1 -D1		Without input pH/ORP Conductivity (SC) Dissolved oxygen (DO)
Output (Note 11)	-A		4-20 mA + HART
—	-N		Always -N
Language set (Note 12)	-LA		English and 11 languages
Country (Note 13)	-N -J		Global except Japan Japan
—	-NN		Always -NN
Option	Mounting hardware Hood Tag plate Conduit adapter	/UM /U /PM /H6 /H7 /H8 /SCT /CB4 /CD4 /CF4	Universal mounting kit (Note 14) Pipe and wall mounting hardware Panel mounting hardware Hood, stainless steel Hood, stainless steel + urethane coating Hood, stainless steel + epoxy coating Stainless steel tag plate Conduit adapter (G1/2 x 4 pcs) Conduit adapter (1/2NPT x 4 pcs) Conduit adapter (M20 x 1.5 x 4 pcs)

Notes:

- 1: The type “-AQ” is General purpose type of EAC. The sales area is limited to Russia.
- 2: The type “-AR” is General purpose type of EAC without any pattern approval for Kazakhstan and Belarus. The sales area is limited to Belarus and Kazakhstan.
- 3: The type “-CB” intrinsic safety type of ATEX and IECEx. Temperature class is T4.
Product registration is done by Yokogawa Taiwan Corporation as an importer in Taiwan.
- 4: The type “-CD” is intrinsic safety of US and Canada, and non-incendive of US and Canada. Temperature classes are T4.
- 5: The type “-CH” intrinsic safety type for NEPSI. Temperature class is T4.
- 6: The type “-EG” intrinsic safety type of KCs for Korea. Temperature class is T4.
- 7: The type “-EQ” intrinsic safety type of EAC with Pattern Approval for Russia. Temperature class is T4. The sales area is limited to Russia.
- 8: The type “-ER” intrinsic safety type of EAC without any pattern approval for Kazakhstan and Belarus. Temperature class is T4. The sales area is limited to Belarus and Kazakhstan.
- 9: The type “-DD” nonincendive type for US. Temperature class is T4.
- 10: When a 2nd input is selected, only the same kind of the 1st input is available.
For example, when a 1st input is “-P1”, the 2nd input must be the same “-P1”.
The combination of ISC and ISC is not available.
- 11: The FLXA21 has other output types of “FOUNDATION Fieldbus” communication (suffix code: -F) and “PROFIBUS PA” communication (suffix code: -P). Refer to GS 12A01A02-71E and GS 12A01A02-72E.


- 12: These languages are message languages on the analyzer's display.
One analyzer has English and 11 languages.
All languages are as follows; English, Chinese, Czech, French, German, Italian, Japanese, Korean, Polish, Portuguese, Russian and Spanish.
- 13: When an analyzer is used in Japan, it must meet the Japanese Measurement Law.
Only SI units must be used on the analyzer and its documents in Japan.
- 14: The universal mounting kit contains the pipe and wall mounting hardware (/U) and the panel mounting hardware (/PM).

■ Dimensions and Mounting

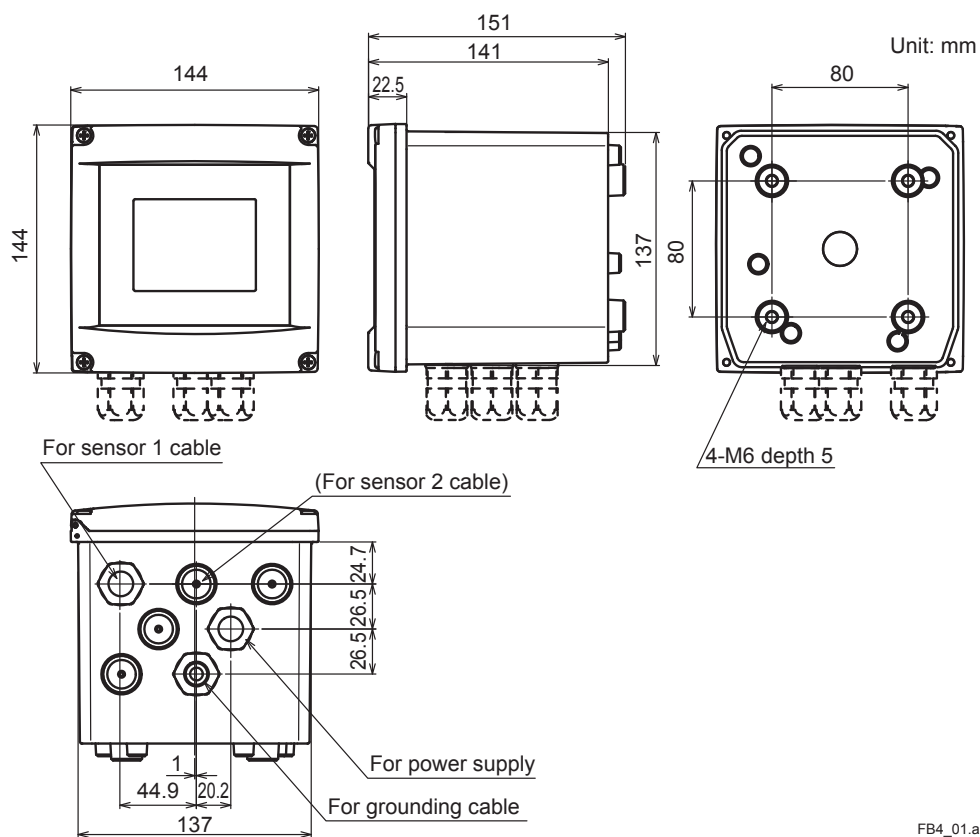


FB4_01.ai

Conduit Adapter (Option code: □/CB4, □/CD4, □/CF4)

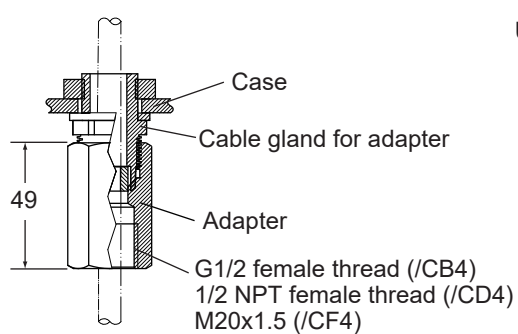


(Note) The universal mounting kit (/UM) contains the pipe and wall mounting hardware (/U) and the panel mounting hardware (/PM).

Panel mounting hardware (Option code: □/PM, □/UM)

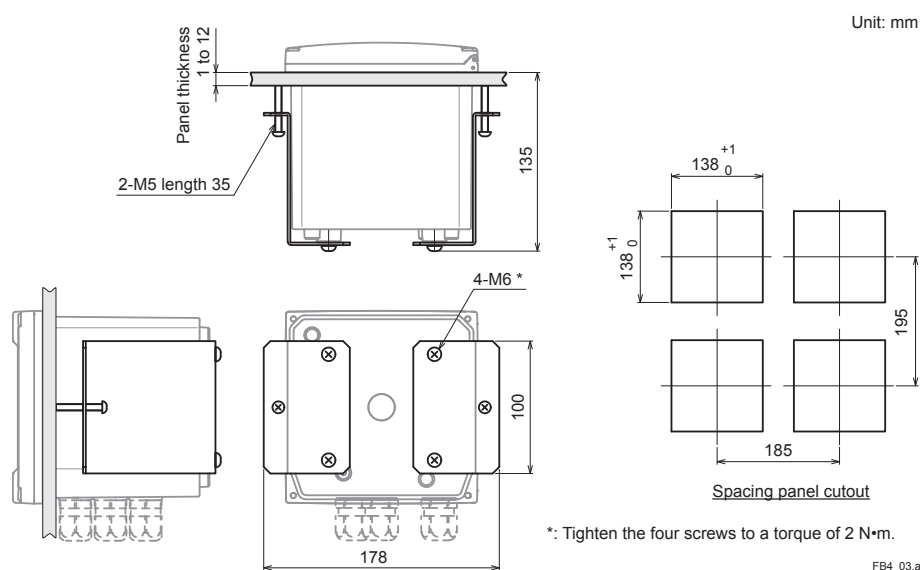



Wall mounting hardware (Option code: □/U, □/UM)

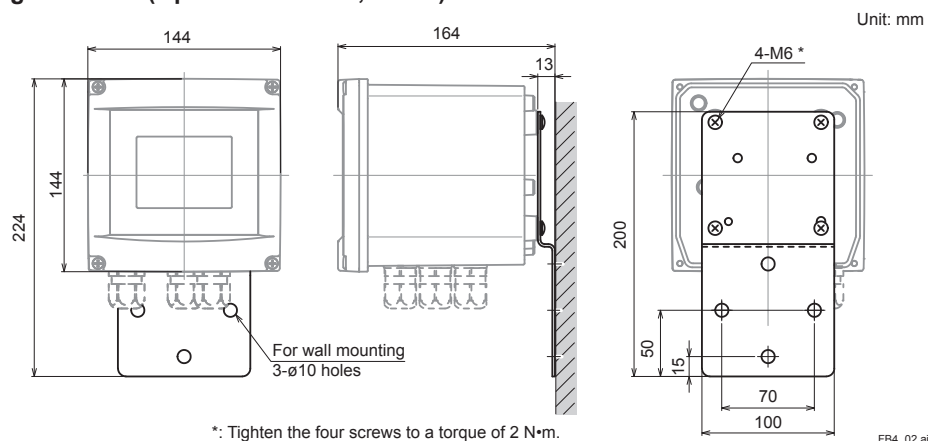


Note: The wall on which the analyzer is mounted should be strong enough to bear the weight of more than 8 kg.

Pipe mounting hardware (Option code: □/U, □/UM)

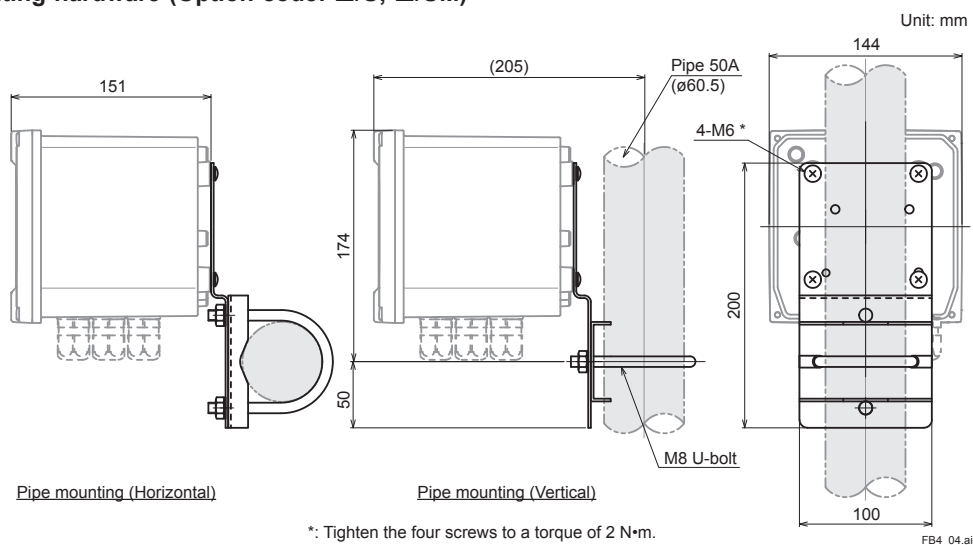


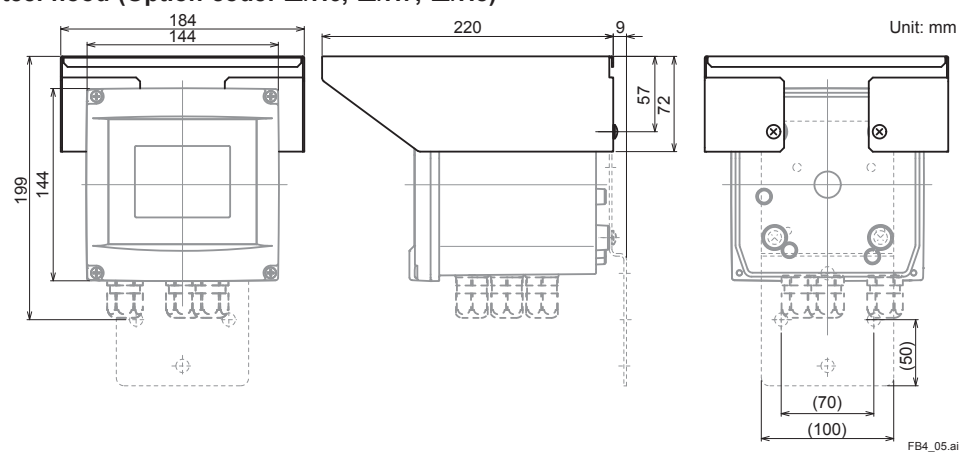Stainless steel hood (Option code: □/H6, □/H7, □/H8)

■ Wiring Diagrams

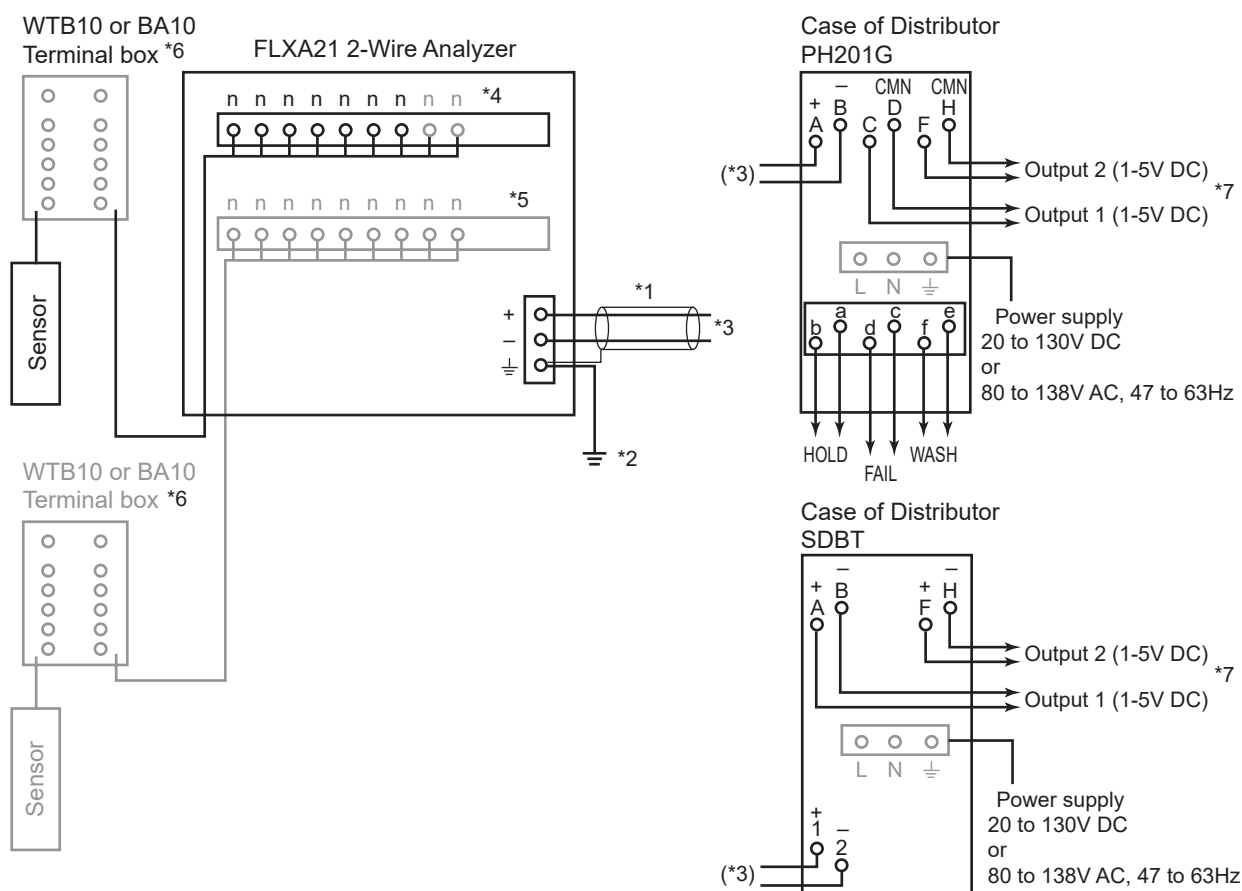

- *1: Use a 2-wire shielded cable with an outside diameter of 6 to 12 mm.
- *2: Connect the analyzer to ground. (Class D ground: 100 ohm or less)
Connect the grounding cable to the $\perp$ terminal of the power module inside.
Use a cable with an outside diameter of 3.4 to 7 mm for the grounding line.
- *3: This line is connected to a distributor or 24V DC power supply.
- *4: Terminal numbers for each sensor module are shown below.
- *5: Two modules of the same kind of measurement/sensor type can be installed. When measuring inductive conductivity, only one module can be installed.
- *6: The terminal box may be necessary depending on the sensor cable length and the distance between the analyzer and the sensor.
- *7: Two outputs, output 1 and output2, of PH201G or SDBT are same signals.

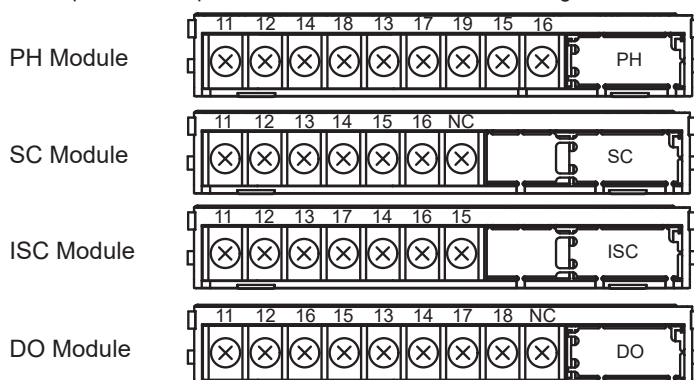

■ Distributor

The distributor PH201G designed exclusively for use with the 2-wire analyzer, supplies drive power to the 2-wire analyzer while simultaneously receiving 4 to 20 mA DC current signal from the analyzer and converting it to 1 to 5 V DC voltage signal; it also simultaneously receives a digital signal superimposed on 4 to 20 mA DC signal, and provides contact outputs during hold, failure, and/or cleaning. A current limiter function is built into the distributor so it can continue to operate properly even with a short circuit on the transmitter side.

● Standard Specifications

<Input/Output Signal Specifications>

Number of input points

(Number of transmitter units connectable): 1 point

Output signal: 1 to 5 V DC (2 points)

Load resistance: 2 kΩ or less (1 to 5 V DC Output)

Isolation system: Loop isolation type

<Mounting/Form>

Mounting method: Indoor rack mounting

Connection method:

External signal connection; M4 screw terminal connection

Power supply/Ground connection:

100 V: JIS C8303 ground type 2 plug connection

220 V: CEE 7VII (European electrical device standard) plug connection

Cable length: 300 mm

External dimensions: 180H x 48W x 300D mm

Weight: Approx. 1.7 kg (Including rack and case)

<Standard Specifications>

Accuracy: ± 0.2 % of span

Analyzer supply voltage: 26.5 ± 1.5 V DC

Insulation resistance

Between I/O terminals and ground pin:

100 MΩ/500 V DC

Between power supply pins and ground pin:

100 MΩ/500 V DC

<Operating Specifications>

Ambient temperature: 0 to 50 °C

Ambient humidity: 5 to 90 % RH (Non-condensing)

Power supply: Dual use AC/DC

100 V: DC power 20 to 130 V, no polarity

AC power 80 to 138 V, 47 to 63 Hz

220 V: DC power 120 to 340 V, no polarity

AC power 138 to 264 V, 47 to 63 Hz

Maximum current and power consumption

24 V DC: Approx. 200 mA

100 V AC: Approx. 7 VA

220 V AC: Approx. 11 VA

<Contact Output>

Contact rating: 250 V AC, maximum 100 VA 220 V DC, maximum 50 VA

Hold contact output: 1 contact, Normally energized
Contact closes when power is off or during maintenance.

Failure contact output: 1 contact, Normally energized
Contact will close when power is off or during the failure.


Cleaning contact output: Close during cleaning only
Used as drive contact for solenoid valve for cleaning.

● Model and Suffix Codes


Model	Suffix Code	Option Code	Specification
PH201G	-----	-----	Distributor
Power Supply	-A1 -A2	----- -----	100V AC version 220V AC version
Style Code	*C	-----	Style C (for FLXA21 & FLXA202)
Option		/TB	Terminal for power connection

- External Dimension

Unit: mm

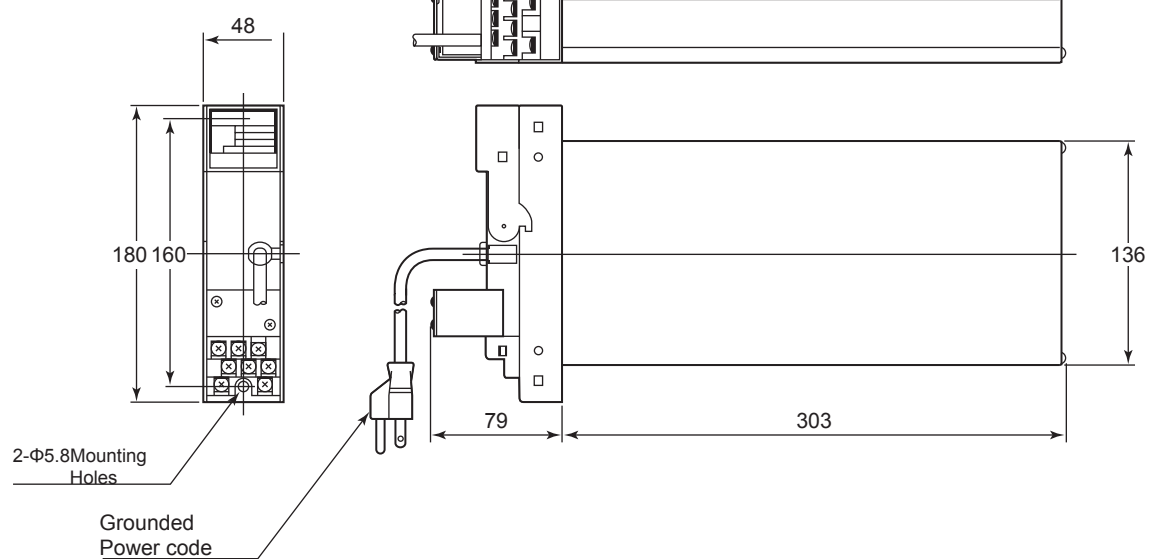**TB with power terminal**

Unit: mm

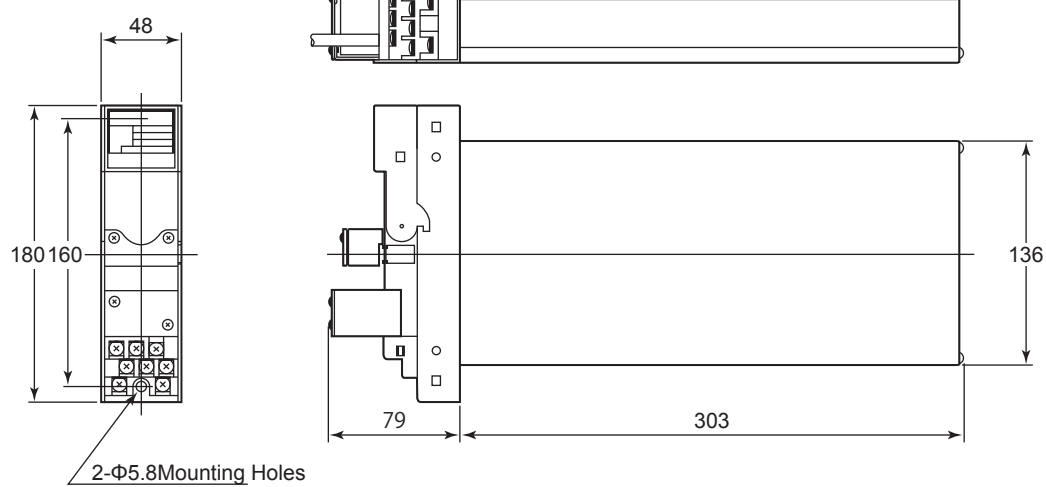

■ Inquiry Specifications Sheet for FLXA21 2-Wire Analyzer

Make inquiries by placing checkmarks (✓) in the pertinent boxes and filling in the blanks.

1. General Information

Company name _____
 Contact Person; _____ Department; _____
 Plant name; _____
 Measurement location; _____
 Purpose of use; ☐ Indication, ☐ Recording, ☐ Alarm, ☐ Control

2. Measurement Conditions

(1) Process temperature; _____ to _____ Normally _____ [°C]
 (2) Process pressure; _____ to _____ Normally _____ [kPa]
 (3) Flow rate; _____ to _____ Normally _____ [l/min]
 (4) Flow speed; _____ to _____ Normally _____ [m/s]
 (5) Slurry or contaminants; ☐ No, ☐ Yes
 (6) Name of process fluid; _____
 (7) Components of process fluid; _____
 (8) Others;

3. Installation Site

(1) Ambient temperature; _____ to _____ [°C]
 (2) Location; ☐ Outdoors, ☐ Indoors
 (3) Others;

4. Requirements

1st Input; ☐ pH/ORP ☐ Conductivity (SC) ☐ Inductive conductivity (ISC)
☐ Dissolved oxygen (DO)
 2nd Input; ☐ With (same as 1st Input) ☐ Without

4.1 pH/ORP

☐ 1st Input

(1) Measuring range; ☐ pH 0 to 14 ☐ ORP _____ to _____ mV ☐ _____
 (2) Transmission output; ☐ 4 to 20 mA DC ☐ pH ☐ ORP ☐ Temperature
 (3) System configuration selection; ☐ Electrode, ☐ Holder, ☐ pH Converter, ☐ Cleaning system, ☐ Terminal box,
☐ Accessories
 (4) Electrode cable length; ☐ 3m, ☐ 5m, ☐ 7m, ☐ 10m, ☐ 15m, ☐ 20m, ☐ _____m
 (5) Electrode operating pressure; ☐ 10 kPa or less, ☐ More than 10 kPa
 (6) Type of holder; ☐ Guide pipe, ☐ Submersion, ☐ Flow-through, ☐ Suspension, ☐ Angled floating ball,
☐ Vertical floating ball
 (7) Cleaning method; ☐ No cleaning, ☐ Ultrasonic cleaning, ☐ Jet cleaning, ☐ Brush cleaning
 (8) Sample temperature; ☐ -5 to 105°C, ☐ -5 to 100°C, ☐ -5 to 80°C
 (9) Others;

☐ 2nd Input

(1) Measuring range; ☐ pH 0 to 14 ☐ ORP _____ to _____ mV ☐ _____
 (2) Transmission output; ☐ 4 to 20 mA DC ☐ pH ☐ ORP ☐ Temperature
 (3) System configuration selection; ☐ Electrode, ☐ Holder, ☐ pH Converter, ☐ Cleaning system, ☐ Terminal box,
☐ Accessories
 (4) Electrode cable length; ☐ 3m, ☐ 5m, ☐ 7m, ☐ 10m, ☐ 15m, ☐ 20m, ☐ _____m
 (5) Electrode operating pressure; ☐ 10 kPa or less, ☐ More than 10 kPa
 (6) Type of holder; ☐ Guide pipe, ☐ Submersion, ☐ Flow-through, ☐ Suspension, ☐ Angled floating ball,
☐ Vertical floating ball
 (7) Cleaning method; ☐ No cleaning, ☐ Ultrasonic cleaning, ☐ Jet cleaning, ☐ Brush cleaning
 (8) Sample temperature; ☐ -5 to 105°C, ☐ -5 to 100°C, ☐ -5 to 80°C
 (9) Others;

4.2 Conductivity

☐ 1st Input

- (1) Measuring range; _____
- (2) Transmission output; 4 to 20 mA DC
- (3) Detector/sensor; SC4AJ ☐ Two electrode system (0.02 cm⁻¹) ☐ Two electrode system (0.1 cm⁻¹)
 SC8SG ☐ Two electrode system (0.01 cm⁻¹) ☐ Two electrode system (10 cm⁻¹),
 ☐ Four electrode system (10 cm⁻¹)
 SC210G ☐ Two electrode system (0.05 cm⁻¹) ☐ Two electrode system (5 cm⁻¹)
- (4) Detector/sensor mounting method;
 SC4AJ ☐ Adapter mounting, ☐ Welding socket, ☐ Welding clamp
 SC8SG ☐ Screw-in, ☐ Flow-through
 SC210G ☐ Screw-in, ☐ Flange, ☐ Flow-through, ☐ Screw-in with gate valve
- (5) Electrode cable length; SC4AJ ☐ 3m, ☐ 5m, ☐ 10m, ☐ 20m
 SC8SG ☐ 5.5m, ☐ 10m, ☐ 20m
 SC210G ☐ 3m, ☐ 5m, ☐ 10m, ☐ 15m, ☐ 20m
- (6) Others;

☐ 2nd Input

- (1) Measuring range; _____
- (2) Transmission output; 4 to 20 mA DC
- (3) Detector/sensor; SC4AJ ☐ Two electrode system (0.02 cm⁻¹) ☐ Two electrode system (0.1 cm⁻¹)
 SC8SG ☐ Two electrode system (0.01 cm⁻¹) ☐ Two electrode system (10 cm⁻¹),
 ☐ Four electrode system (10 cm⁻¹)
 SC210G ☐ Two electrode system (0.05 cm⁻¹) ☐ Two electrode system (5 cm⁻¹)
- (4) Detector/sensor mounting method;
 SC4AJ ☐ Adapter mounting, ☐ Welding socket, ☐ Welding clamp
 SC8SG ☐ Screw-in, ☐ Flow-through
 SC210G ☐ Screw-in, ☐ Flange, ☐ Flow-through, ☐ Screw-in with gate valve
- (5) Electrode cable length; SC4AJ ☐ 3m, ☐ 5m, ☐ 10m, ☐ 20m
 SC8SG ☐ 5.5m, ☐ 10m, ☐ 20m
 SC210G ☐ 3m, ☐ 5m, ☐ 10m, ☐ 15m, ☐ 20m
- (6) Others;

4.3 Inductive conductivity

- (1) Measuring range; _____
- (2) Transmission output; 4 to 20 mA DC
- (3) System configuration selection; ☐ ISC40GJ Sensor, ☐ Holder, ☐ Converter, ☐ BA20 Terminal box,
 ☐ WF10J Extension cable
- (4) Sensor mounting method; ☐ ISC40FDJ Immersion holder, ☐ ISC40FFJ Flow-through holder,
 ☐ ISC40FSJ Direct insertion adapter
- (5) ISC40GJ Sensor cable length; ☐ 5m, ☐ 10m, ☐ 15m, ☐ 20m
- (6) WF10J Extension cable length; ☐ 5m, ☐ 10m, ☐ 20m, ☐ 30m, ☐ 40m
- (7) Others;

(1) Measuring range; ☐ 0 to 50 mg/L ☐ _____

(2) Transmission output; 4 to 20 mA DC

(3) System configuration selection; ☐ Electrode, ☐ Holder, ☐ Converter, ☐ Cleaning system,
☐ Terminal box, ☐ Maintenance parts set, ☐ Calibration set

(4) Electrode cable length; ☐ 3m, ☐ 5m, ☐ 10m, ☐ 15m, ☐ 20m

(5) Type of holder; ☐ Guide pipe, ☐ Submersion, ☐ Flow-through, ☐ Suspension,
☐ Angled floating ball, ☐ Vertical floating ball

(6) Cleaning method; ☐ No cleaning, ☐ Jet cleaning

(7) Others;

(1) Measuring range; ☐ 0 to 50 mg/L ☐ _____

(2) Transmission output; 4 to 20 mA DC

(3) System configuration selection; ☐ Electrode, ☐ Holder, ☐ Converter, ☐ Cleaning system,
☐ Terminal box, ☐ Maintenance parts set, ☐ Calibration set

(4) Electrode cable length; ☐ 3m, ☐ 5m, ☐ 10m, ☐ 15m, ☐ 20m

(5) Type of holder; ☐ Guide pipe, ☐ Submersion, ☐ Flow-through, ☐ Suspension,
☐ Angled floating ball, ☐ Vertical floating ball

(6) Cleaning method; ☐ No cleaning, ☐ Jet cleaning

(7) Others;